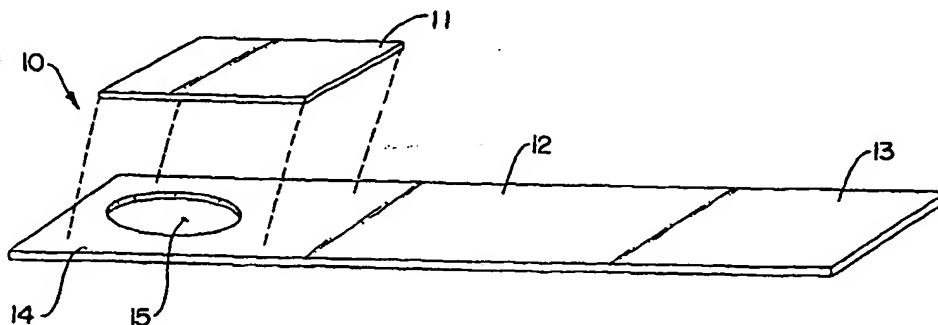




INTERNATIONAL APPLICATION PUBLISHED UNDER THE PATENT COOPERATION TREATY (PCT)

(51) International Patent Classification ⁷ : G01N 33/52, A61B 10/00	A1	(11) International Publication Number: WO 00/39579 (43) International Publication Date: 6 July 2000 (06.07.00)
<p>(21) International Application Number: PCT/US99/31129</p> <p>(22) International Filing Date: 29 December 1999 (29.12.99)</p> <p>(30) Priority Data: 09/222,123 29 December 1998 (29.12.98) US</p> <p>(71) Applicant: FLEXSITE DIAGNOSTICS, INC. [US/US]; 3543 S.W. Corporate Parkway, Palm City, FL 34990 (US).</p> <p>(72) Inventors: RAY, Robert, A.; 815 S.W. Rustic Circle, Stuart, FL 34990 (US). LUI, May, S.; 6688 110th Street, Sebastian, FL 32948 (US). SUMMERS, Susan; 4203 S.E. Jacaranda Street, Stuart, FL 34997 (US). SMITH, Brian; 589 S.W. Ray Avenue, Port St. Lucie, FL 34983 (US).</p> <p>(74) Agents: STEELE, J., Rodman, Jr. et al.; Quarles & Brady LLP, Suite 400, 222 Lakeview Avenue, P.O. Box 3188, West Palm Beach, FL 33402-3188 (US).</p>		<p>(81) Designated States: AE, AL, AM, AT, AU, AZ, BA, BB, BG, BR, BY, CA, CH, CN, CU, CZ, DE, DK, EE, ES, FI, GB, GE, GH, GM, HR, HU, ID, IL, IS, JP, KE, KG, KP, KR, KZ, LC, LK, LR, LS, LT, LU, LV, MD, MG, MK, MN, MW, MX, NO, NZ, PL, PT, RO, RU, SD, SE, SG, SI, SK, SL, TJ, TM, TR, TT, UA, UG, UZ, VN, YU, ZA, ARIPO patent (GH, GM, KE, LS, MW, SD, SL, SZ, TZ, UG, ZW), Eurasian patent (AM, AZ, BY, KG, KZ, MD, RU, TJ, TM), European patent (AT, BE, CH, CY, DE, DK, ES, FI, FR, GB, GR, IE, IT, LU, MC, NL, PT, SE), OAPI patent (BF, BJ, CF, CG, CI, CM, GA, GN, GW, ML, MR, NE, SN, TD, TG).</p> <p>Published <i>With international search report. Before the expiration of the time limit for amending the claims and to be republished in the event of the receipt of amendments.</i></p>

(54) Title: REMOTE SITE URINE COLLECTION DEVICE AND METHOD OF USE



(57) Abstract

A device for collecting, drying, and transporting a urine sample, and extracting an analyte of interest from the dried sample for determining the presence or absence of the analyte or, if present, the amount or concentration thereof, is described. A preferred embodiment of the device is a sample collection strip which includes a collection pad for collecting and retaining the sample and a handle member for handling or manipulation of the device. Methods of use, and kits relating to the device are also described.

FOR THE PURPOSES OF INFORMATION ONLY

Codes used to identify States party to the PCT on the front pages of pamphlets publishing international applications under the PCT.

AL	Albania	ES	Spain	LS	Lesotho	SI	Slovenia
AM	Armenia	FI	Finland	LT	Lithuania	SK	Slovakia
AT	Austria	FR	France	LU	Luxembourg	SN	Senegal
AU	Australia	GA	Gabon	LV	Latvia	SZ	Swaziland
AZ	Azerbaijan	GB	United Kingdom	MC	Monaco	TD	Chad
BA	Bosnia and Herzegovina	GE	Georgia	MD	Republic of Moldova	TG	Togo
BB	Barbados	GH	Ghana	MG	Madagascar	TJ	Tajikistan
BE	Belgium	GN	Guinea	MK	The former Yugoslav Republic of Macedonia	TM	Turkmenistan
BF	Burkina Faso	GR	Greece	ML	Mali	TR	Turkey
BG	Bulgaria	HU	Hungary	MN	Mongolia	TT	Trinidad and Tobago
BJ	Benin	IE	Ireland	MR	Mauritania	UA	Ukraine
BR	Brazil	IL	Israel	MW	Malawi	UG	Uganda
BY	Belarus	IS	Iceland	MX	Mexico	US	United States of America
CA	Canada	IT	Italy	NE	Niger	UZ	Uzbekistan
CF	Central African Republic	JP	Japan	NL	Netherlands	VN	Viet Nam
CG	Congo	KE	Kenya	NO	Norway	YU	Yugoslavia
CH	Switzerland	KG	Kyrgyzstan	NZ	New Zealand	ZW	Zimbabwe
CI	Côte d'Ivoire	KP	Democratic People's Republic of Korea	PL	Poland		
CM	Cameroon	KR	Republic of Korea	PT	Portugal		
CN	China	KZ	Kazakstan	RO	Romania		
CU	Cuba	LC	Saint Lucia	RU	Russian Federation		
CZ	Czech Republic	LI	Liechtenstein	SD	Sudan		
DE	Germany	LK	Sri Lanka	SE	Sweden		
DK	Denmark	LR	Liberia	SG	Singapore		
EE	Estonia						

REMOTE SITE URINE COLLECTION DEVICE
AND METHOD OF USE

Background of the Invention

5 Analysis of biological fluids has long been used for diagnosing disease or metabolic disorders of living organisms. Blood and urine have been a primary source for obtaining biological components from animals, especially humans, for conducting such analyses. While blood components can be useful for determining a range of information about the health condition of an animal, 10 obtaining a blood sample is still considered invasive. Thus, collection of urine, and analysis of certain components contained therein, can be advantageous for determining the health status of an animal, especially those which may be at risk of developing, or have developed, nephropathies or other renal, urinary, or metabolic disorders.

15 There are multiple renal disease etiologies in which laboratory findings include proteinuria. Albumin is the prominent protein in most renal diseases. Micro-albuminuria refers to albumin concentration in urine which is greater than normal, but usually not detectable with routine protein dipstick assays which permit measurement of albumin of 15 mg/dL or greater. Monitoring low 20 concentrations of albumin in the urine is helpful for early detection of nephropathy in patients at risk for renal disease.

 Those at risk for renal disease in which albuminuria may be present include, but are not limited to, patients with Type I and Type II diabetes, hypertension, and renal disease in pregnancy.

25 Of all patients beginning therapy for end-stage renal disease in the United

States, diabetic nephropathy is the major cause of renal failure in twenty-five percent. Recent studies of the natural history of patients with long standing diabetes showed that microalbuminuria preceded clinical diabetic nephropathy. Further studies indicate that normalization of blood glucose and blood pressure
5 can prolong the progression from microalbuminuria to clinical nephropathy.

Rapid tests have been developed for on-site urinalysis. For example, Boehringer Mannheim Corporation (Indianapolis, Indiana, USA) manufactures Micral™ urine test strips, a semi-quantitative microalbuminuria test for early detection of subclinical nephropathy. However, this test involves binding of the
10 urine albumin with a specific antibody-gold conjugate which is present on the strip. Albumin content is determined by a color change when a conjugate-albumin immunocomplex is formed. One disadvantage of this test, like other immunoassays, is that the determination must be made at the time of testing. According to the product literature or "label," the color reaction must be
15 determined within five minutes of color development because the immunocomplex (and color change) disintegrates thereafter.

Another product available from Boehringer Mannheim Corporation is Chemstrip® which is a rapid multi-parameter test strip which is used to measure certain constituents in urine, including specific gravity, pH, leukocytes, nitrite,
20 protein, glucose, ketones, urobilinogen, bilirubin, blood, and hemoglobin, which are useful in the evaluation of renal, urinary, and metabolic disorders. This test also involves a color change directly on the strip which is compared to a standardized color chart for component measurement. However, this Chemstrip® product is also limited in its long-term stability after contact with

urine. The color changes which are used in determining results are stable only about 120 seconds after immersion. The product labeling indicates that "[c]olor changes that occur after 2 minutes from immersion are not of clinical value."

On-site rapid tests which use a color change for determining measurement
5 of urine components can also be less precise and less accurate than
conventional laboratory testing of those components. One reason is that the
user, unfamiliar with standard laboratory or medical diagnostic procedures, may
not fully appreciate the need for accurately following the prescribed testing
procedure. Even minor deviation from the prescribed protocol can affect results
10 and, hence, diagnosis.

Heretofore, remote-site sampling of urine, i.e., collection of a urine sample
for transport to and analysis in a laboratory, was limited to collection of a liquid
sample. The limitations and disadvantages of collection and transport of liquid
samples are obvious and include the need to collect minimum volumes, as well
15 as the risks of contamination, breakage, spillage, or degradation.

A need thus exists for a device and method for remote-site collection of a
urine sample which provides for the sample to be transported in a dry state for
subsequent urinalysis in a laboratory. Ideally, such a device and method would
provide for collecting minimum volumes which can be standardized for precise
20 and accurate analysis, as well as reducing the risk of contamination and
eliminate the risk of spillage or degradation.

Brief Summary of the Invention

The subject invention concerns a device and method for collection,

stabilization, preservation, transport, storage, processing, and compatibility with laboratory analysis of a biological sample obtained from a living organism. In particular, the subject invention concerns a device and method used in the collection and analysis of a component in a urine sample obtained from an animal. Methods and kits are also described for use of the subject device.

The subject invention provides for a device which is useful for collecting a urine sample from an animal, e.g., a human, drying of the urine sample on the device, transporting the collected and dried urine sample to a laboratory or other facility for analysis, and eluting or extracting an analyte of interest from the dried sample for determining the presence or absence of the analyte or, if present, the amount or concentration thereof.

One embodiment of the subject device is a collection strip which comprises a non-reactive collection pad for collecting and retaining a urine sample containing an analyte of interest, and a handle member on which the collection pad can be disposed whereby the handle member can facilitate handling or manipulation of the device without the user having to directly contact the collection pad. Preferably, the handle member is an elongate strip of material, e.g., high impact polystyrene, which is rigid enough to prevent drooping or bending of the handle member in normal use. The strip forms a handle end by which the user can hold the device, and a collection end which provides an area for disposing the collection pad.

In a preferred embodiment, the collection pad comprises an absorbent, sponge-like material which can readily absorb the liquid urine sample. The collection pad functions to retain the sample and its components in an unreacted

state, even when the sample is dried. Advantageously, the collection pad allows for high-recovery extraction of the dried sample, or an analyte therein, for subsequent laboratory analysis. The collection pad can be a polymeric material, e.g., polyvinyl alcohol, or glass fiber, cellulose, or the like. In addition, the
5 collection pad can be treated with a preservative for preventing premature breakdown or denaturation of the analyte of interest, or with a blocking agent which can prevent irreversible binding of an analyte of interest so that recovery of the analyte is maximized.

The collection pad can be a separate member affixed to the collection end
10 of the strip or can be made integral with the strip. Preferably, the handle member and collection pad form a unitary device for collecting and processing of the sample. The device can be made to provide a means for separating or removing at least a portion of the collection pad from the strip.

One embodiment providing a removable portion of the collection pad
15 includes a collection pad permanently affixed to one face of the strip wherein the collection end of the strip has an opening or aperture therethrough, over which the collection pad is affixed. This apertured configuration of the collection end of the strip provides at least partial exposure of the face of the collection pad contacting the strip. A portion of the collection pad can then be
20 separated from the remainder of the pad by a hole punching apparatus or other cutting means which can remove a portion of predetermined size from the pad. The removal of a portion of the collection pad having a predetermined size can be useful for collection and extraction of consistent amounts of sample.

In use, the subject device is provided as a unitary sample collection strip

or "dipstick" comprising the handle member and collection pad. The urine sample can be applied to the collection pad, e.g., by holding the strip at the handle end and contacting the collection pad with a liquid urine sample to saturate the collection pad. The pad is then allowed to dry, is packaged for shipping, and is transported, typically by mail, to a laboratory for analysis. The analysis is performed by removing a predetermined sized portion of the collection pad, performing an extraction method to recover an analyte of interest from the collection pad, and determining presence or absence of the analyte or, if present, measuring an amount or concentration of the analyte. The results of the analysis can then be reported to a physician and/or the patient.

The manufacture of the subject device comprises providing an elongate strip of a relatively rigid material, e.g., a plastic or polymeric material, which has a handle end serving as a handle for holding and manipulating the device, and a collection end which provides a substrate for a urine collection pad. An opening can be formed through the strip at the collection end by punching or cutting the strip.

The collection pad comprises a relatively flat section of absorbent, sponge-like material, and can be shaped as desired. Typically, the collection pad is a square, substantially equal or slightly smaller in width than the width of the strip. After forming the opening in the collection end of the strip, the collection pad can be affixed or adhered to one face of the strip, in a position and being of relative size to completely cover the opening.

Preferably, the collection pad can be affixed to the strip by applying appropriate amounts of heat and pressure so that adhesion forms between the

pad and strip materials. Alternatively, the collection pad can be ultrasonically welded to the strip, adhered by applying a compatible adhesive between the pad and strip, or affixed by a mechanical fastening means.

Multiple strips can be manufactured by providing a sheet of strip material which is cut to length of the strips. Openings can be formed at one end of the sheet at appropriate positions for forming multiple strips. A strip of collection pad material can then be applied over the openings, and the sheet can be cut into individual strips.

Brief Description of the Drawings

Fig. 1 Shows an exploded perspective view of one embodiment of the device according to the subject invention.

Fig. 2 shows a configuration for making multiple strips from a single sheet of strip material.

Fig. 3 shows an embodiment of the device according to the subject invention comprising a plurality of collection pads disposed on the strip.

Figs. 4A-4D show results of testing a device according to the subject invention for percent recovery of analyte in samples spiked with known concentrations of albumin. Fig. 4A shows recovery of known standards from a neat sample (i.e., not applied to the device); Fig. 4B shows recovery from an undried collection pad; Fig. 4C shows recovery from a collection pad dried overnight at room temperature; and Fig. 4D shows recovery from a collection pad dried overnight at room temperature and at 45 degrees C for two days.

Figs. 5A-5C show results of a correlation study using a device according

to the subject invention over a range of albumin concentrations (measured as a ratio of microalbumin to creatinine) at increasing drying times versus neat samples (unapplied to the device). Fig. 5A shows microalbumin/creatinine ratios for 1 day drying at room temperature; Fig. 5B shows microalbumin/creatinine ratios for 4 day drying at room temperature; and Fig. 5C shows microalbumin/creatinine ratios for 7 day drying at room temperature.

Fig. 6 shows stability testing of a device according to the subject invention measured as microalbumin/creatinine ratios at room temperature at 0, 1, 4, and 7 days drying time.

Fig. 7 shows results from a comparative study between two polymeric hydrogel materials, namely, Merocel® and Clinichel®, at different drying times and temperatures.

Detailed Description of the Preferred Embodiments

The subject invention concerns a device and method for collection, stabilization, preservation, transport, storage, processing, and compatibility with laboratory analysis of a biological sample obtained from a living organism. In particular, the subject invention concerns a device and method used in the collection and analysis of a component in a urine sample obtained from an animal.

The subject device can be understood by reference to the accompanying drawings. Figure 1 shows an embodiment of the subject device which is useful for collecting a urine sample from an animal, e.g., a human, drying of the urine sample on the device, transporting the dried collected urine sample to a

laboratory or other facility for analysis, and eluting or extracting an analyte of interest from the sample for determining the presence or absence of the analyte or, if present, the amount or concentration thereof.

Specifically, Figure 1 shows a device 10 according to the subject
5 invention comprising non-reactive collection pad 11 for collecting and retaining a urine sample containing an analyte of interest, and a handle member or strip 12 to facilitate handling of the device without contacting the collection pad. Preferably, the handle member 12 is an elongate strip of material, e.g., high impact polystyrene, which is rigid enough to prevent drooping or bending of the
10 handle member in normal use. Typically, the strip forming the handle member is a polystyrene material about 2 mm in thickness. This thickness retains rigidity of the strip and allows for a hole punching apparatus to be used to remove a portion of the collection member. It would be understood that other materials can be used for the strip so long as the material performs the stated functions of
15 the device and is compatible with the collection pad material and with urine.

The strip of material forms a handle end 13 by which the user can hold the device, and a collection end 14 which provides an area for disposing of the collection pad. In a preferred embodiment, the collection pad comprises an absorbent, sponge-like material which can readily absorb the liquid urine sample.
20 The collection pad functions to retain the sample and its components in an unreacted state, even when the sample is dried. Advantageously, the collection pad allows for high-recovery extraction of the dried sample, or an analyte therein, for subsequent laboratory analysis.

The collection pad can be a polymeric material, preferably a hydrogel

material, e.g., polyvinyl alcohol, or glass fiber, cellulose, or the like, or can be a mixture of materials. Polyvinyl alcohol (PVA) materials which can be used for the collection pad are Merocel®, available from Merocel Scientific Product, Inc. (Mystic, Connecticut, USA) or Clinical®, available from M-Pact (Endora, Kansas, USA). Merocel® and Clinical® are available in varying pore sizes and densities. For example, the densities of Merocel® range from about 0.049 to about 0.1 g/cc, dry. The pore sizes range from about 0.01 to about 1.2 mm.

A preferred Merocel® product for use in the subject invention is marketed as "CF-100" which has the following properties: density (dry, g/cc) -- 0.067; average pore size -- 0.45 mm; pore size range -- 0.02-0.6 mm; void volume 93%; absorbency time -- < 5 seconds; absorptive capacity (g water/ g sponge) -- 16X; retained capacity (g water/ g sponge) -- 12X; tensile strength -- 46 psi; and percent elongation -- 210.

The collection pad is preferably substantially non-reactive in that there is no reagent, indicator, or other component included in the pad which provides for rapid, on-site determination or measurement of analyte. For example, the subject invention does not include a pad which changes color according to exposure to varying amounts of analyte so that the patient can immediately determine results. However, the collection pad can be treated with a preservative for preventing premature degradation or denaturation of the analyte of interest, or can be treated with a blocking agent which can prevent irreversible binding of an analyte of interest to facilitate recovery thereof. A preferred blocking agent for use in determining microalbumin concentrations is bovine serum albumin (BSA). The preferred pretreatment comprises saturating

the collection pad in a 500-1000 mg/L solution of BSA in 0.1M Tris (pH 7.6), then allowing the pad to dry.

The collection pad is shown as a separate member affixed to the collection end on a top face of the strip. Regardless of the way in which the collection pad is affixed to the strip it is preferable that the handle member and collection pad form a unitary device for collecting and processing of the sample. As further illustrated in Figure 1, a means for providing a removable portion of the collection pad 11 can include providing an opening or aperture 15 through the collection end 14 of the strip. The collection pad is affixed onto the strip 12, over the aperture 15 at the collection end 14. This aperture 15 formed in the collection end 14 of strip 12 provides at least partial exposure of the face of the collection pad contacting the strip.

A portion of the collection pad can then be separated from the remainder of the pad by a hole punching apparatus or other cutting means which can remove a predetermined sized portion of from the pad. It would be understood that the collection pad can alternatively be pre-scored with a die-cut or perforation to facilitate separation and removal of the predetermined sized portion, or that a predetermined sized collection pad can be removably affixed to or made removably integral with the handle component. The predetermined size of the removable portion of the collection pad provides for collection and extraction of consistent amounts of sample or analyte.

In use, the subject device is provided as a unitary sample collection strip or "dipstick" comprising the handle member and collection pad. The urine sample can be applied to the collection pad by direct exposure during urination

or, preferably, can be applied by holding the strip at the handle end and dipping the collection end comprising the collection pad into a liquid urine sample which has been collected or placed in a container. The collection pad is allowed to become saturated with sample. Such "dipstick" procedures are well-known in the art.

Once the urine sample is saturated onto the collection pad, the pad is allowed to dry for at least one to two hours, and preferably overnight. The device can then be packaged for shipping and transported, typically by mail, to a laboratory for analysis.

The urinalysis is performed by removing the predetermined sized portion of the collection pad and performing an extraction method to recover an analyte of interest from the collection pad. Typically, the removed portion of the collection pad is placed into a container and eluted with water or aqueous buffer solution to extract the analyte from the collected sample. The presence or absence of the analyte can then be determined or, if present, the amount or concentration measured, by standard procedures which are well known in the art. The determination or measurement is preferably made by a commercially available automated analyzer. The results of the analysis can then be reported to a physician and/or the patient.

Advantageously, the subject device provide for near 100% recovery of analyte when tested using a control solution to which a known concentration of analyte has been added or "spiked." Recoveries are consistently greater than 60% and, on average, are approximately 80% or greater when tested on the day following overnight drying. Recovery of analyte from a clinical sample is

considered to be comparable. The subject device can be used for determination or measurement of all analytes commonly assayed in urinalysis panels performed by clinical laboratories. Primarily, however, the subject invention is useful for determining presence or absence or measuring low concentrations of urinary albumin (microalbumin). In addition, the subject device can be advantageous for determining presence or absence or measuring metabolites indicative of osteoporosis, e.g., pyrilinks-D or N-telopeptides.

The manufacture of the subject device comprises providing an elongate strip of a relatively rigid material, e.g., a plastic or polymeric material, which has a handle end serving as a handle for holding and manipulating the device, and a collection end which provides a support layer for a urine collection pad. The dimensions of the strip are not critical so long as they allow for performing all necessary functions as described herein. For example, the length of the strip should be of sufficient length to facilitate handling of the device without requiring the user to directly contact the collection pad. Any contact of the collection pad in the collection process can contaminate the sample and can be contrary to good hygiene practices once the collection pad is saturated with urine. Typically, the strip is about four inches in length and about 3/4 inches in width which allows the user to easily dip the device into a urine sample collected into a standard collection cup.

The thickness of the strip should provide a relatively rigid device so that the strip does not droop or bend in use. In addition, it can be advantageous for drying if the strip can be rigid enough to be laid across the top of the urine sample collection cup during the drying process. On the other hand, the

thickness of the strip should not be such that it does not fit between the working ends of a standard hole punching apparatus or is too thick to be easily punched by a punch press. Typically, a polystyrene material of about 2mm in thickness is sufficient to meet these requirements.

5 An opening 15 through the strip at the collection end can be formed by cutting the strip, preferably centrally punching out a generally circular or ovoid section from the collection end so that the face of the collection pad contacting the strip is exposed when disposed onto the strip. The opening should preferably be larger than the predetermined sized portion of the collection pad
10 which is removable from the device. A preferred size for the opening is therefore greater than 1/4 inch and is typically about 7/16 inches in diameter. Exposure of the contact face of the collection pad can be advantageous for thorough drying of the collection pad and for accessing the collection pad with a hole punching apparatus for removing a predetermined sized portion of the pad.
15 The predetermined size of the removable portion of the collection pad is preferably approximately 3/16-1/4 inch in diameter so that a minimum amount of sample required for testing can be absorbed into and recovered from the collection pad.

 The collection pad comprises a relatively flat section of absorbent,
20 sponge-like material, and can be shaped as desired. Typically, the collection pad is a square, substantially equal or slightly smaller in width than the width of the strip, and is of standard thickness as is commercially available for the material. After forming the opening in the collection end of the strip, the collection pad can be affixed or adhered to one face of the strip, in a position and being of

relative size to completely cover the opening. Preferably, the collection pad can be affixed to the strip by applying appropriate amounts of heat and pressure so that adhesion forms between the pad and strip materials. Alternatively, the collection pad can be ultrasonically welded to the strip, adhered by applying a compatible adhesive between the pad and strip, or affixed by a mechanical fastening means.

As shown in Fig. 2, multiple strips can be manufactured by providing a sheet 22 of strip material which is cut to length of the strips, preferably about four inches. Openings 23 can be formed at one end, referred to herein as the collection end 24, of the sheet at appropriate positions for forming multiple strips. A strip of collection pad material 25 can then be applied over the openings, and the sheet can be cut into individual strips, shown by the dotted lines.

It would also be understood by persons of ordinary skill in the art, in view of the disclosure herein, that other embodiments are contemplated for the subject device. One of these alternative embodiments is shown in Fig. 3, which provides a device according to the subject invention having a plurality of collection pads disposed thereon for collecting separate or multiple samples from a single urine specimen.

The embodiment shown in Fig. 3 comprises two separate collection pads and two apertures formed in the collection end of the strip. In addition, the collection pads and apertures are shown aligned along a longitudinal axis of the strip. It would be understood that more than two collection pads can be

provided on a

single strip and that the plurality of collection pads can alternatively be aligned side-by-side on the collection end of the strip.

The subject invention further concerns a kit for enabling an individual to collect a sample and transport the collected sample to a facility for analysis. in general, the kit, comprising at least one of the above-described devices and instructions for use of the device, can further include separately packaged components selected from the following: sterile urine collection cup, transport packaging, or an information card for providing information, e.g., medical history or health status of the individual being tested for disease or metabolic disorder.

Following are examples which illustrate procedures for practicing the invention. These examples should not be construed as limiting.

Example 1 -- Recovery of Urinary Albumin

To determine recovery of albumin added to normal urine, a device according to a preferred embodiment of the subject invention, namely a 3/4" X 4" X 2mm strip having a 3/4" X 3/4" Merocel® collection pad disposed thereon, was saturated by dipping the device into a urine sample spiked with either 10, 50, 100 or 200mg/dL albumin.

Testing was done on a neat sample of urine (i.e., collected sample which was not applied to the subject device), on samples applied to and extracted from the collection pad of the subject device, ten minutes following application of urine to the collection pad, on samples extracted following drying, overnight at room temperature on the collection pad, as well as samples collected following

drying overnight at room temperature then at 45 degrees C for two days to simulate mailing conditions. The results are shown in Figs. 4A-4D and indicate greater than 60% recovery for all conditions and from 96-104% recovery after 10 minutes drying time on the collection pad. The greater than 100% recovery was likely due to a concentration phenomenon.

Example 2 -- Correlation of Collected Urinary Albumin to Neat Sample

Correlation and stability of albumin collected onto an embodiment of the subject device as described in Example 1 was tested over a range of albumin concentrations (measured as a ratio from 0 to 3 of microalbumin to creatinine) at increasing drying times versus neat samples (samples unapplied to the device). The results of these tests are shown in Figs. 5A-5C. Each of the tests demonstrates excellent correlation with a neat sample for up to 7 days of drying time. Microalbumin/creatinine ratios for 1, 4, and 7 days drying at room temperature show greater than 99% correlation ($R^2 = 0.99$ or greater) as shown in Figs. 5A-5C.

Stability testing of the device described in Example 1 was measured as microalbumin/creatinine ratios at room temperature at 0, 1, 4, and 7 days drying time for multiple samples. Samples collected on the subject device showed excellent stability for up to 7 days drying time (Fig. 6).

Example 3 -- Comparison of Polyvinyl Alcohol Materials

A comparative study between two polymeric hydrogel materials, namely, Merocel® and Clinichel®, at different drying times and temperatures was

conducted to determine potential differences in materials used for the collection pad of the subject device. Neat samples applied to each of the materials were tested along with samples collected after 1 day drying time at room temperature, after 3 days drying time at 45° C, and after 7 days drying time at room temperature. As shown in Fig. 7, stability of microalbumin/creatinine ratios over time was comparable for each of the materials.

Microalbumin/creatinine ratios for Merocel® ranged from 0.692 to 0.745, compared to a ratio of 0.657 for the neat sample. Microalbumin/creatinine ratios for Clinichel® ranged from 0.64 to 0.71 compared to a ratio of 0.65 for the neat sample.

It should be understood that the examples and embodiments described herein are for illustrative purposes only and that various modifications or changes in light thereof will be suggested to persons skilled in the art and are to be included within the spirit and purview of this application and the scope of the appended claims.

Claims

What is claimed is:

- 1 1. A device for remote-site collection and drying of a liquid biological
2 sample obtained from an individual for the purpose of mailing the dried sample
3 for recovery and laboratory analysis of an analyte contained in the biological
4 sample, said device comprising:
5 a relatively rigid strip forming a handle member having a handle end
6 and a collection end, said collection end having a collection pad for collecting
7 and drying the sample containing the analyte, said collection pad capable of
8 having at least a portion thereof removed from the device to recover the analyte
9 for detection or measurement by laboratory analysis.
- 1 2. The device of claim 1 wherein the biological sample is urine.
- 1 3. The device of claim 1 wherein the analyte is albumin.
- 1 4. The device of claim 1 wherein the collection pad is an absorbent
2 material.
- 1 5. The device of claim 4 wherein the collection pad material is
2 selected from hydrogel, glass fiber, glass fiber/cellulose mixtures, or cellulose.
- 1 6. The device of claim 5 wherein the hydrogel is polyvinyl alcohol.

1 7. The device of claim 1 wherein the strip has an aperture formed in
2 the collection end which exposes a portion of a face of the collection pad
3 contacting the strip.

1 8. The device of claim 1 wherein the collection pad is pre-treated with
2 a reagent which facilitates the collection, separation, storage, transport,
3 preservation, recovery, or analysis of the sample.

1 9. The device of claim 8 wherein the collection pad pre-treatment
2 reagent is a solution comprising bovine serum albumin.

1 10. The device of claim 1 wherein the collection pad is substantially
2 non-reactive for purposes of providing a rapid, on-site diagnostic test.

1 11. The device of claim 1 wherein said device comprises a plurality of
2 collection pads.

1 12. The device of claim 1 wherein said device comprises a plurality of
2 apertures formed in the collection end of the strip.

1 13. A method for remote-site collection of a biological sample and
2 laboratory analysis of an analyte in the sample, said method comprising:
3 providing a collection device to an individual or a health care
4 professional, said device comprising a relatively rigid strip forming a handle

5 member having a handle end and a collection end, said collection end having a
6 collection pad for collecting and drying the sample containing the analyte, said
7 collection pad capable of having at least a portion thereof removed from the
8 device to recover the analyte for detection or measurement by laboratory
9 analysis;

10 applying the biological sample in liquid form to the device so that
11 the analyte-containing component of interest is collected onto the collection pad;
12 drying said collection pad having the analyte-containing component
13 of interest retained therein;

14 transporting the device to a facility for analysis of the analyte;
15 removing at least a portion of the collection pad from the device;
16 eluting the analyte from the collection pad;
17 determining presence, absence, or concentration of the analyte; and
18 reporting results of the analysis to the individual or health care
19 professional.

1 14. The method of claim 13 wherein the drying step is completed
2 before the step of removing at least a portion of the collection pad.

1 15. The method of claim 13 further comprising identifying the individual
2 and sample by a code.

1 16. The method of claim 13 wherein the elution step is modified
2 according to the particular analyte being determined or measured.

1 17. The method of claim 13 wherein the step of determining presence,
2 absence, or measuring of the analyte is modified according to said analyte.

1 18. The method of claim 13 wherein the collection pad is substantially
2 non-reactive for purposes of providing a rapid, on-site diagnostic test.

1 19. A kit for remote-site collecting of a biological sample from a patient
2 for laboratory analysis of said sample, said kit comprising:

3 a sample collection device comprising a relatively rigid strip forming
4 a handle member having a handle end and a collection end, said collection end
5 having a collection pad for collecting and drying the sample containing the
6 analyte, said collection pad capable of having at least a portion thereof removed
7 from the device to recover the analyte for detection or measurement by
8 laboratory analysis; and

9 an information card for providing information about the patient.

1 20. The kit of claim 19 wherein said kit further comprises a component
2 selected from a urine collection cup, and packaging means for transporting the
3 collected sample.

1/7

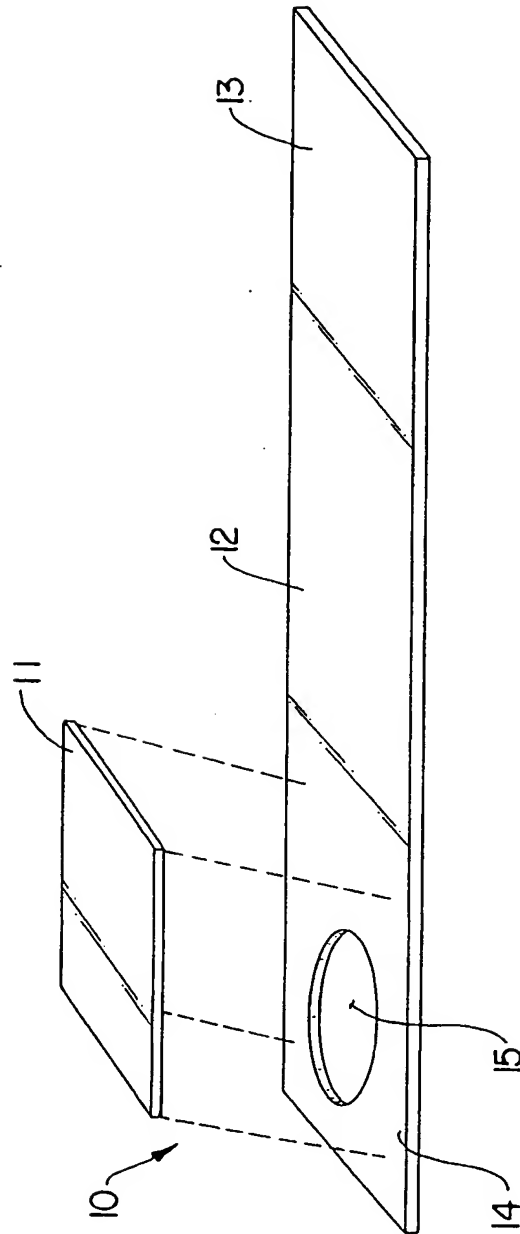


FIG. 1

2/7

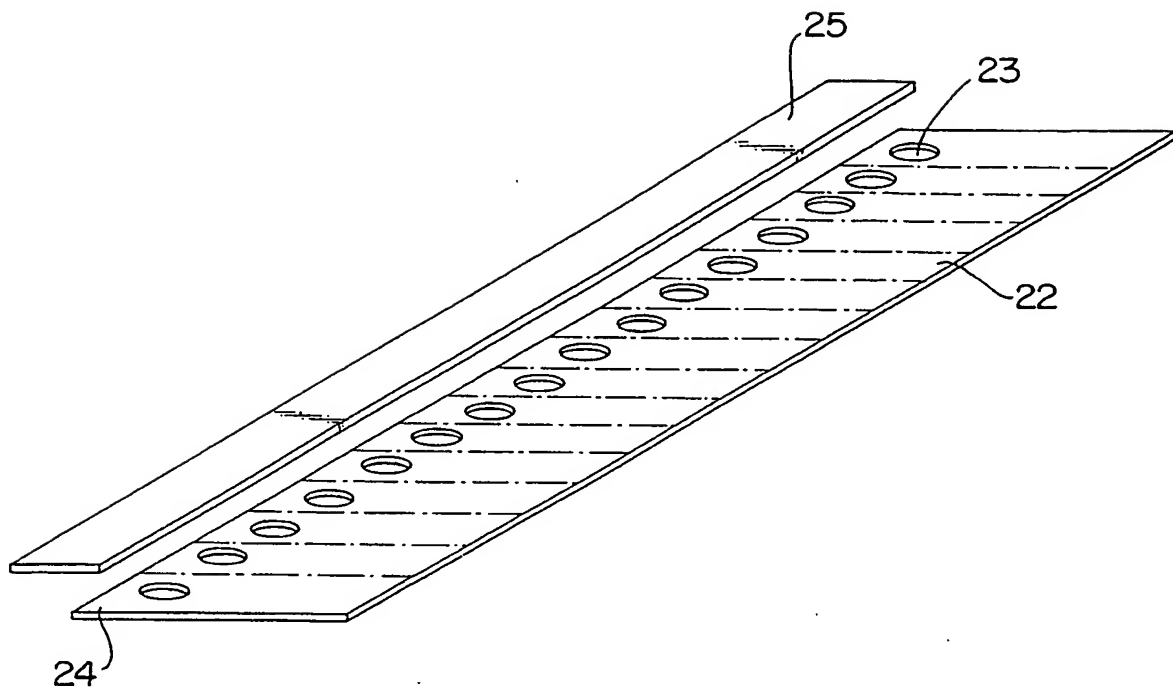


FIG. 2

3/7

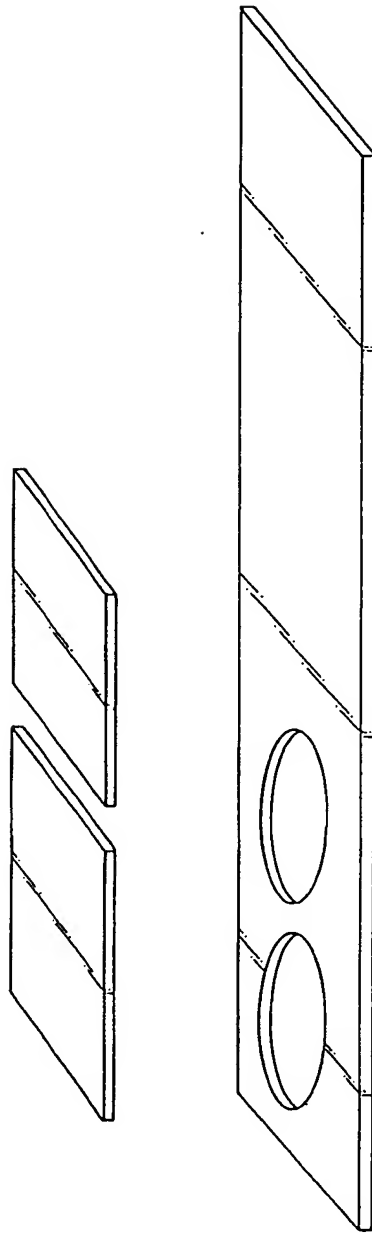


FIG. 3

4/7

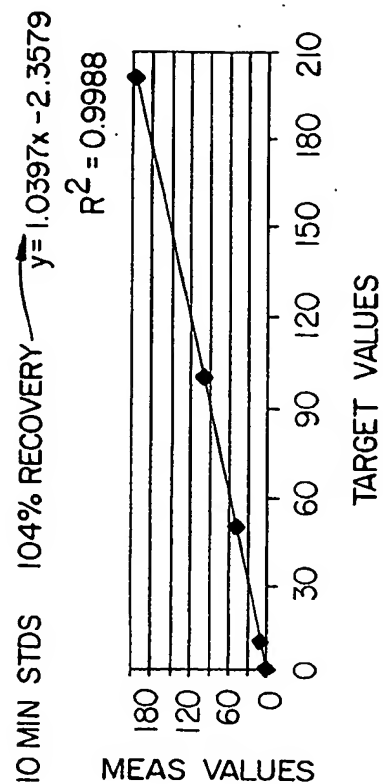


FIG. 4B

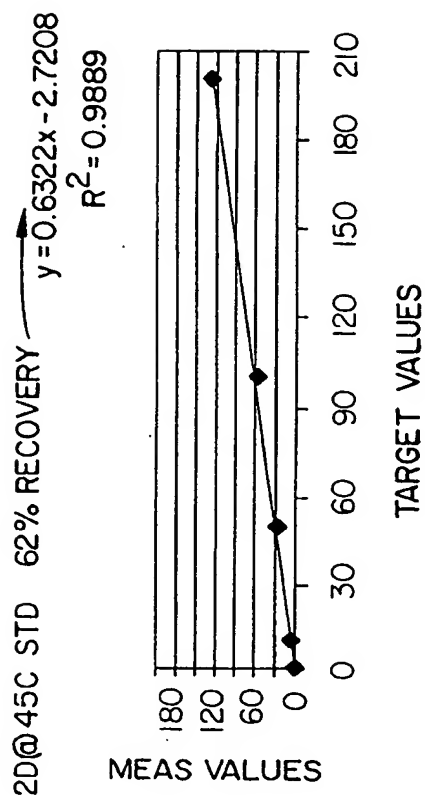


FIG. 4D

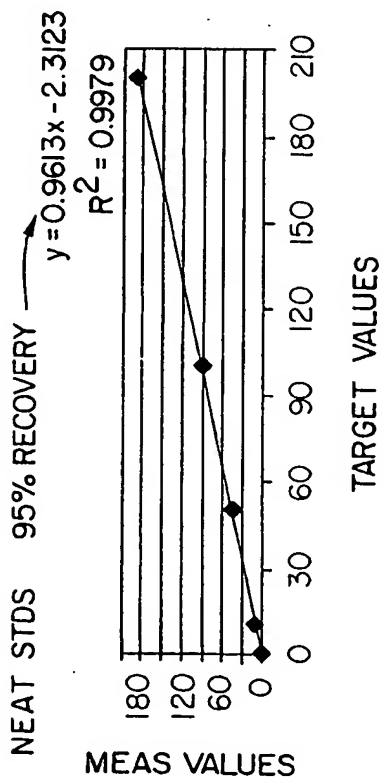


FIG. 4A

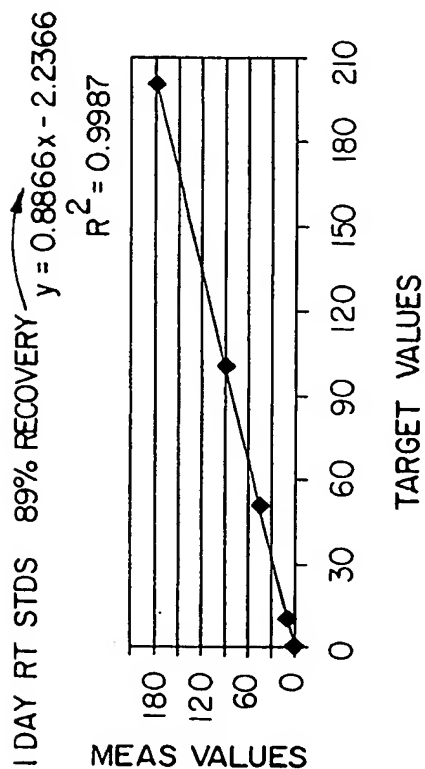
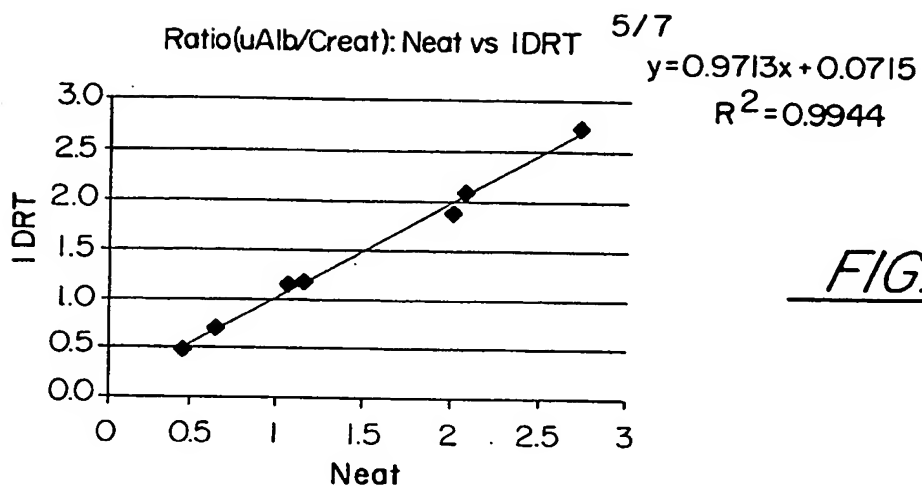
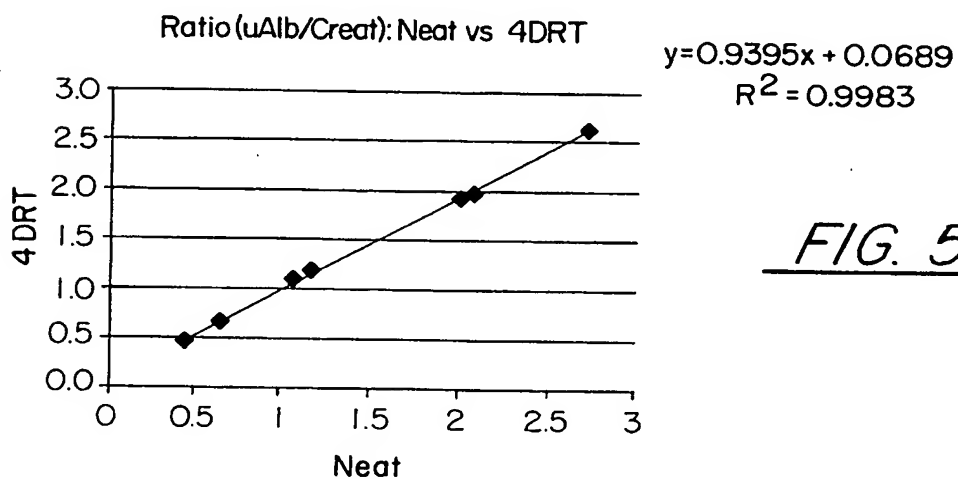
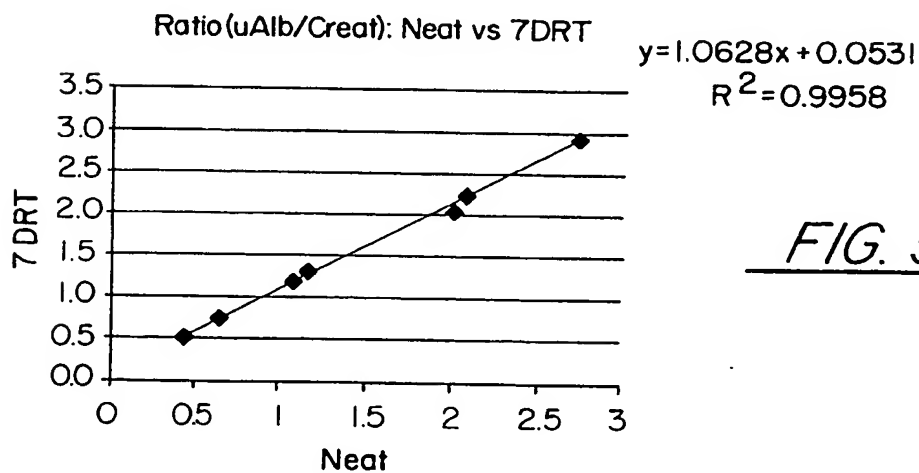
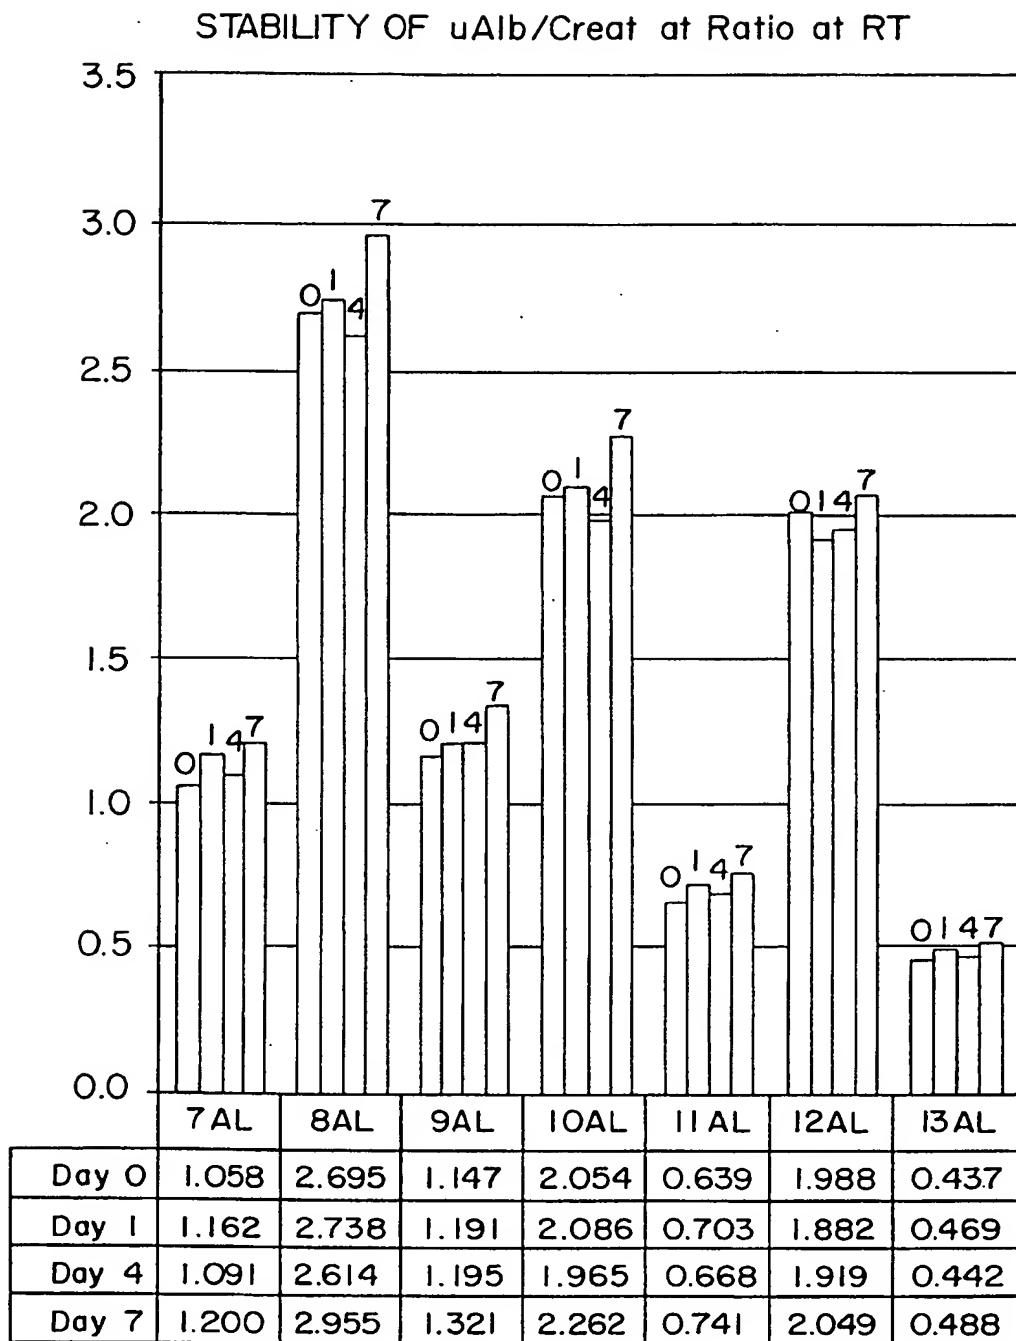


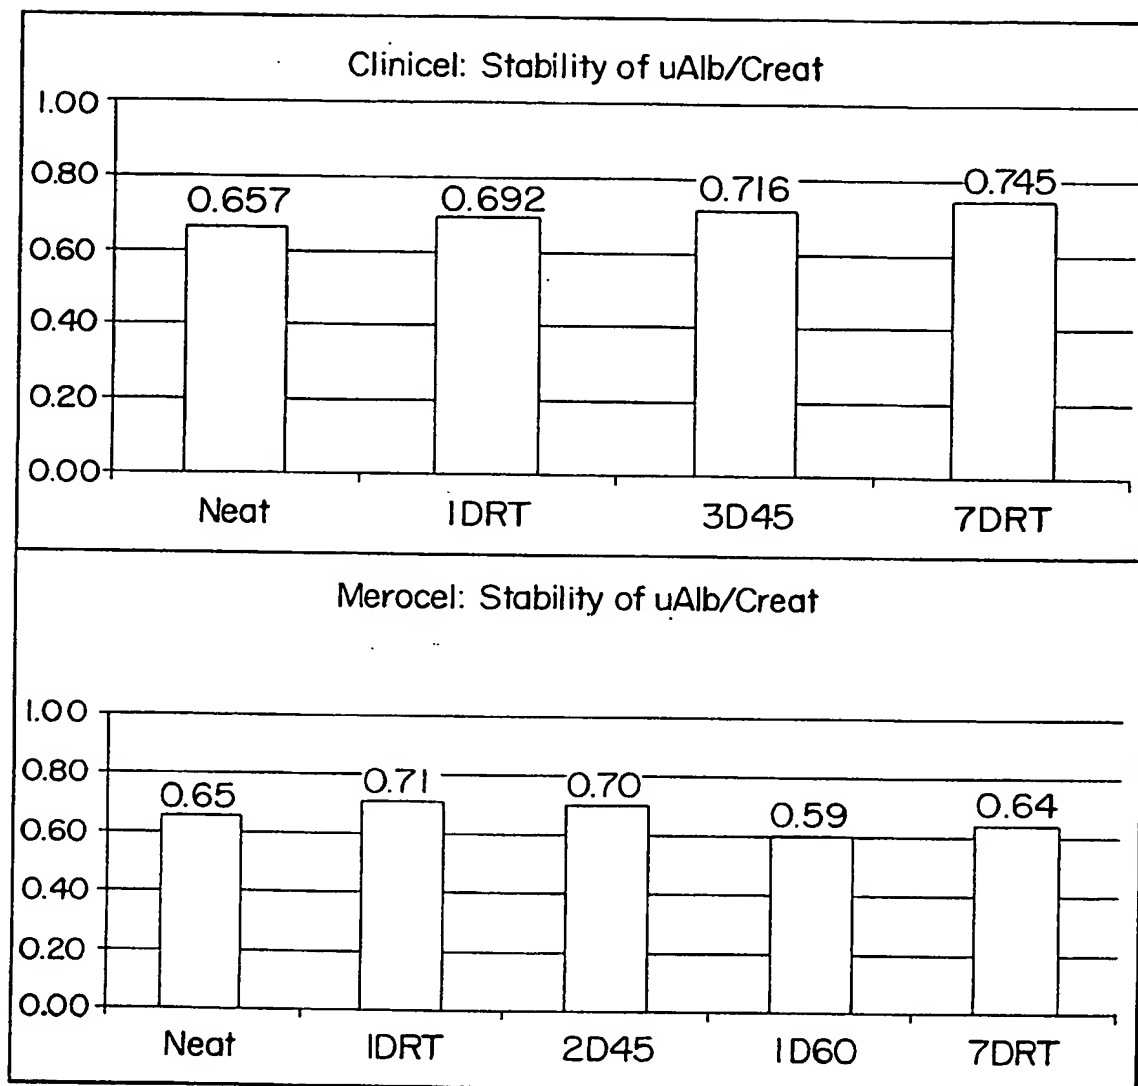
FIG. 4C

FIG. 5AFIG. 5BFIG. 5C

6/7

FIG. 6

7/7

FIG. 7

INTERNATIONAL SEARCH REPORT

Int. National Application No.

PCT/US 99/31129

A. CLASSIFICATION OF SUBJECT MATTER
IPC 7 G01N33/52 A61B10/00

According to International Patent Classification (IPC) or to both national classification and IPC

B. FIELDS SEARCHED

Minimum documentation searched (classification system followed by classification symbols)

IPC 7 G01N A61B

Documentation searched other than minimum documentation to the extent that such documents are included in the fields searched

Electronic data base consulted during the International search (name of data base and, where practical, search terms used)

C. DOCUMENTS CONSIDERED TO BE RELEVANT

Category *	Citation of document, with indication, where appropriate, of the relevant passages	Relevant to claim No.
X	EP 0 734 686 A (ORTHO PHARMACEUTICAL CORPORATION) 2 October 1996 (1996-10-02)	1,4,7,8,
Y	the whole document	13-20
X	WO 97 19754 A (BOEHRINGER MANNHEIM GMBH.)	1,13,19
Y	5 June 1997 (1997-06-05)	1-20
X	WO 93 11434 A (OSBORN LABORATORIES, INC.)	1,13,19
	10 June 1993 (1993-06-10)	
	abstract	
X	WO 95 27205 A (EPITOPE, INC.)	1,13,19
	12 October 1995 (1995-10-12)	
	abstract	

	---/--	

☒ Further documents are listed in the continuation of box C.☒ Patent family members are listed in annex.

* Special categories of cited documents :

"A" document defining the general state of the art which is not considered to be of particular relevance

"E" earlier document but published on or after the international filing date

"L" document which may throw doubts on priority claim(s) or which is cited to establish the publication date of another citation or other special reason (as specified)

"O" document referring to an oral disclosure, use, exhibition or other means

"P" document published prior to the international filing date but later than the priority date claimed

"T" later document published after the international filing date or priority date and not in conflict with the application but cited to understand the principle or theory underlying the invention

"X" document of particular relevance; the claimed invention cannot be considered novel or cannot be considered to involve an inventive step when the document is taken alone

"Y" document of particular relevance; the claimed invention cannot be considered to involve an inventive step when the document is combined with one or more other such documents, such combination being obvious to a person skilled in the art.

"A" document member of the same patent family

Date of the actual completion of the international search

10 May 2000

Date of mailing of the international search report

24/05/2000

Name and mailing address of the ISA

European Patent Office, P.B. 5818 Patentlaan 2
NL - 2280 HV Rijswijk
Tel. (+31-70) 340-2040, Tx. 31 651 epo nl,
Fax: (+31-70) 340-3016

Authorized officer

Griffith, G

INTERNATIONAL SEARCH REPORT

In *donal* Application No

PCT/US 99/31129

C.(Continuation) DOCUMENTS CONSIDERED TO BE RELEVANT

Category *	Citation of document, with indication, where appropriate, of the relevant passages	Relevant to claim No.
X	WO 96 28715 A (H. M. CHANDLER) 19 September 1996 (1996-09-19) the whole document	1,13,19
Y	DE 35 06 365 A (DAI NIPPON INSATSU K.K.) 29 August 1985 (1985-08-29) claims; figures	1-20
Y	US 5 443 080 A (J. P. D'ANGELO) 22 August 1995 (1995-08-22) the whole document	1-20
Y	EP 0 022 377 A (R. A. LEVINE) 14 January 1981 (1981-01-14) the whole document	1-20

INTERNATIONAL SEARCH REPORT

Information on patent family members

International Application No

PCT/US 99/31129

Patent document cited in search report		Publication date	Patent family member(s)	Publication date
EP 734686	A	02-10-1996	US 5609160 A AU 5038896 A BR 9601190 A CA 2172764 A CN 1142354 A CZ 9600934 A HU 9600818 A JP 8320278 A PL 313508 A	11-03-1997 10-10-1996 31-03-1998 01-10-1996 12-02-1997 16-10-1996 28-07-1997 03-12-1996 14-10-1996
WO 9719754	A	05-06-1997	AU 7697396 A CA 2238763 A EP 0863802 A US 5895704 A	19-06-1997 05-06-1997 16-09-1998 20-04-1999
WO 9311434	A	10-06-1993	US 5334502 A CA 2121361 A,C EP 0625268 A	02-08-1994 10-06-1993 23-11-1994
WO 9527205	A	12-10-1995	US 5714341 A AT 175274 T AU 2197595 A DE 69507019 D EP 0753148 A	03-02-1998 15-01-1999 23-10-1995 11-02-1999 15-01-1997
WO 9628715	A	19-09-1996	AU 700777 B AU 4871296 A CA 2215346 A EP 0815424 A JP 11502018 T ZA 9601950 A	14-01-1999 02-10-1996 19-09-1996 07-01-1998 16-02-1999 06-11-1996
DE 3506365	A	29-08-1985	JP 1934225 C JP 6053074 B JP 60178356 A US 5183742 A	26-05-1995 20-07-1994 12-09-1985 02-02-1993
US 5443080	A	22-08-1995	US 5462064 A	31-10-1995
EP 0022377	A	14-01-1981	US 4259964 A AT 12697 T DE 3070449 D JP 1630824 C JP 2057669 B JP 56053445 A US 4273741 A US 4559949 A	07-04-1981 15-04-1985 15-05-1985 26-12-1991 05-12-1990 13-05-1981 16-06-1981 24-12-1985